


US

UNITED STATES PATENT AND TRADEMARK OFFICE

I, Michael J. WALSH, European Patent Attorney, of the firm of Tomkins & Co., Chartered Patent Agents and European Patent Attorneys, of 5 Dartmouth Road, Dublin 6, Ireland, declare;

1. That I am a citizen of The Republic of Ireland.
2. That I am well acquainted with the German and English languages.
3. That the attached is, to the best of my knowledge and belief, a true translation into the English language of an Official Certificate of the German Patent Office dated 2 February 2004 and of the text of a copy of the specification of German Patent Application No. 101 37 011.3 attached thereto.
4. That I believe that all statements made herein of my own knowledge are true and that all statements made on information and belief are true; and further that these statements were made with the knowledge that willful false statements and the like so made are punishable by fine or imprisonment, or both, under Section 1001 of Title 18 of the United States Code and that such willful false statements may jeopardize the validity of the patent application in the United States of America or any patent issuing thereon.


MICHAEL J. WALSH

The 7th day of July 2005

DE

FEDERAL REPUBLIC OF GERMANY

(eagle insignia)

Priority Certificate for the Filing of a Patent Application

File Number: 101 37 011.3

Date of Application: 28 July 2001

Applicant/Owner: Aesculap AG & Co KG
78532 Tuttlingen/Germany

Title: Medical Implant System

IPC: A 61 B 17/68

The attached copies are a correct and exact reproduction of the original documents of this patent application.

Munich, 2 February 2004

The German Patent and Trademark Office,

The President,

By order

(signature)

MJW10308

MEDICAL IMPLANT SYSTEM

The invention relates to a medical implant system with an implant made of a composite material in which glass
5 fibers are embedded.

Medical implants, for example bone plates, intramedullary nails, endoprotheses, osteosynthesis systems for the spinal column, etc., are usually
10 produced from metal materials, but there are also known implants which consist of a composite material in which glass fibers are embedded for reinforcement; in particular, such medical implants consist of selected sterilizable plastics, such as polyether ether ketone,
15 polyamides, etc.

When these implants are inserted into the body, they are subjected to various influences, for example various stresses and strains, temperature developments
20 or chemical environments. It would be of interest to the doctor carrying out the procedure to find out about these different parameters, since they provide information on how healing progresses or on problems possibly occurring.

25 It is an object of the invention to improve an medical implant system of the generic type in such a way that information on physical properties in the implant and in its environment can be obtained.

30 In the case of a medical implant of the type described at the beginning, this object is achieved according to the invention by a sensor element which is embedded in the implant and comprises at least one of the glass
35 fibers being connected to a measuring device which determines a physical property of the sensor element or its environment and changing of this property.

Consequently, at least one glass fiber embedded in the composite material of the implant is used for the transmission of signals which provide information on the physical properties of the implant or the
5 environment of the implant.

In this case, the term "glass fiber" is understood as meaning all fibrous substances which can be embedded in the composite material and are capable of carrying and
10 transmitting electromagnetic radiation; these fibers preferably consist of quartz glass, but other substances may also be used, for example synthetic fibers, known as Plastic Optical Fibers (POFs).

15 It is advantageous if the glass fibers are embedded in the composite material as mechanical reinforcement.

In particular, it may be provided in this case that the glass fibers are arranged in the form of a woven
20 fabric, a knitted fabric or a non-woven fabric, that is to say form a mesh which is embedded as a whole in the composite material and reinforces the latter as a result.

25 Depending on the mechanical requirements, the glass fibers may in this case be concentrated in specific regions of the implant, or else be distributed over the entire extent of the implant.

30 The measuring device is preferably formed in such a way that it feeds electromagnetic radiation into the sensor element and determines physical properties of the sensor element or of its environment from the type of radiation that passes through and/or is reflected.

35 According to a preferred embodiment, the glass fiber of the sensor element is provided with a radiation-reflecting coating.

In the case of a first preferred embodiment, the sensor element substantially consists of the glass fiber forming a sensor fiber. In the case of this
5 embodiment, the glass fiber embedded in the composite material is consequently at the same time the sensor and transmission element for the electromagnetic radiation.

10 Quite a large number of different configurations in which the glass fiber acts as a sensor fiber are possible, for example at least one region acting as a Bragg grating may be incorporated in the sensor fiber. In such a region, which has periodic changes of the
15 refractive index in the longitudinal direction of the sensor fiber, radiation is reflected, said radiation being superposed during the reflection and only intensifying in the return direction for quite specific wavelengths. This wavelength depends on the
20 periodicity of the Bragg grating region and changes with this periodicity. Any change in length of the sensor fiber or any change in the periodicity of the Bragg grating that occurs on account of external influences can in this way be detected in the form of a
25 wavelength shift.

In the case of another preferred embodiment, it may be provided that a substance which is induced to fluoresce by the fed-in electromagnetic radiation and the
30 fluorescent properties of which undergo changes under the effect of the environment outside the sensor fiber is embedded in the sensor fiber. These changes may be mechanical changes, but the fluorescent property of the embedded substance can in particular be influenced by
35 the chemical environment of the sensor fiber, for example the fluorescence can be extinguished by certain substances in the environment.

In the case of a further preferred embodiment, it is provided that the radiation-reflecting coating consists of a substance which changes the reflection behavior for the electromagnetic radiation in the sensor fiber under the effect of the environment outside the sensor fiber. As a result, the amount of radiation that passes through and is reflected by the sensor fiber changes, and this can be detected.

Every change of the properties in the radiation can be detected; this may comprise changes of the wavelength, of the phase position, of the polarization, etc., but all that is important is that these changes are in a clearly perceivable relationship with changes of the properties in the environment of the sensor fiber, that is to say for example with changes of the mechanical stress, the temperature or the material composition.

In the case of a further preferred embodiment, it may be provided that the sensor element comprises the glass fiber and a further sensor member which is connected to the measuring device via the glass fiber. In the case of this configuration, the glass fiber acts substantially as a transmission element between the sensor member and the measuring device.

For example, the sensor member may be a pressure sensor with a flexible membrane and a mirror element which can be moved by the latter and reflects the electromagnetic radiation fed into the glass fiber differently according to position.

In the case of a further embodiment, the sensor member may be a Fabry-Pérot interferometer.

For example, it may in this case be provided that the Fabry-Pérot interferometer is formed as a thin-film interferometer that is brought into contact onto and at

the end of the glass fiber and the active film of which undergoes dimensional changes under the influence of the environment. Such an active film may, for example, be in a porous form and swell when it comes into
5 contact with a liquid; in this way it is possible for example to detect whether an implant is still sealed or has a desired or undesired opening with respect to the environment.

10 In the case of another embodiment, it is provided that the Fabry-Pérot interferometer comprises two glass fibers with polished end faces, the spacing between which can be changed by environmental influences. This configuration is advantageous in particular whenever
15 strains or displacements within an implant are to be detected.

The glass fiber of the sensor element may be connected directly to the measuring device, it being possible for
20 the measuring device to be carried inside the body, but also outside it. In the latter case, the glass fiber is led out from the implant through the body tissue, so that a connection to the measuring device can be established there.

25 It is particularly advantageous if the measuring device is a microcontroller that is capable of being implanted in the body.

30 In the case of a particularly preferred embodiment, the glass fiber is connected to a transducer, which exchanges signals with the measuring device without a physical connection.

35 This transducer may in particular be capable of being implanted in the body, for example it may be a transponder.

In the case of a particularly advantageous embodiment, the transducer is a light source which has an associated light receiver. It has been found that light of different wavelengths can penetrate body
5 tissue to a certain extent, with the result that a transmission of radiation energy is possible by light between a light receiver and a light source, of which one component is disposed in the body and one component outside it, in particular whenever the light source
10 emits electromagnetic radiation in the range between 650 and 1000 nm.

In the case of a particularly preferred embodiment, associated with the measuring device is a radiation
15 transmitter, which transports radiation into the interior of the implant via a glass fiber in the implant. In addition to determining the physical properties of the implant by the coupled-in radiation, such a radiation transmitter can be used for acting on
20 the implant and changing it, for example by heating it up in specific regions or the like.

It may in this case be provided that the transport of the radiation takes place via a glass fiber which is
25 embedded in the implant in addition to the glass fiber of a sensor element, but it may also be provided that the transport of the radiation takes place via the glass fiber of a sensor element. In this case, it is advantageous to use appropriate switching elements that
30 selectively connect the glass fiber to the measuring device and to the radiation transmitter.

Particularly advantageous is a configuration in which the wavelength and intensity of the transported
35 radiation are chosen such that the radiation induces mechanical and/or material changes in the composite material of the implant. For example, it is possible in this way to perform additional hardening of a

polymeric composite material in specific regions or, conversely, weakening by destroying the composite material, with the result that the mechanical properties of the implant can be changed in this way in
5 relatively large areas or else locally.

In the case of a particularly preferred embodiment, it is provided in this case that associated with the measuring device and the radiation transmitter is a
10 controller, which activates the radiation transmitter in dependence on the measured values of the measuring device. In the case of this configuration, it is possible to determine the physical data of the implant continuously, for example the mechanical stresses
15 transferred to the implant, which are for example a measure of the healing process; these stresses decrease with increasing stability at the bone connection, since a part of the loads are taken over by the bone. It is then advantageous to reduce the strength of the implant
20 corresponding to this regeneration of the bone connection, with the result that the force-transfer function is increasingly taken over by the healing bone.

25 The following description of preferred embodiments of the invention serves for a more detailed explanation in conjunction with the drawing, in which:

Figure 1 shows a schematic view of an implant in the
30 form of a bone plate with a wireless connection to a measuring device;

Figure 2 shows a schematic view of an implant in the
35 form of a plate with a glass fiber reinforcement in the form of a mesh;

Figure 3 shows a schematic view of an implant in the form of a bone plate with a measuring device

connected to a number of glass fibers and with a radiation source for the introduction of radiation into a glass fiber that is not connected to the measuring device;

5

Figure 4 shows a view similar to Figure 3 with a switching device for the selective connection of glass fibers in the implant to the measuring device or to the radiation source;

10

Figure 5 shows a schematic side view of a glass fiber with Bragg grating regions of different periodicity;

15

Figure 6 shows a schematic side view of a glass fiber with embedded fluorescent dye particles;

20

Figure 7 shows a schematic side view of a glass fiber with a sheathing having changeable transmission properties;

25

Figure 8 shows a schematic side view of a Fabry-Pérot interferometer connected to a glass fiber, with two pieces of glass fiber that are moved towards each other;

Figure 9 shows a view similar to Figure 8 with a dimensionally-changeable active film, and

30

Figure 10 shows a schematic side view of a glass fiber with a membrane pressure sensor.

35

The invention is explained below on the basis of the example of a bone plate; however, it is to be understood however that the invention can be used generally for medical implants that can be inserted in the body and is not restricted to bone plates.

An implant 1 in the form of a bone plate with openings 2 for receiving bone screws is connected in a way known per se by means of bone screws to two bone fragments 3, 4 in such a way that the latter are fixed in a specific relative position with respect to each other, with the result for example that a fracture 5 can heal (figure 1). The implant 1 consists of a synthetic material, for example a resorbable plastic such as polyactide (PLLA, PL DLLA), polyglycolide (PGA) or trimethylene carbonate (TMC), and glass fibers 7 are embedded in this synthetic material 6. In the exemplary embodiment of Figure 1, only two individual glass fibers 7 are schematically represented, extending in the longitudinal direction of the plate-shaped implant 1; in the exemplary embodiment of Figure 2, a multiplicity of glass fibers 7 are indicated in the form of a mesh, which is embedded as a whole in the synthetic material 6; the widest variety of arrangements and concentrations of glass fibers in the synthetic material 6 are possible here. The glass fibers reinforce the synthetic material 6 by this embedding, and different distributions in the implant are accordingly chosen, depending on the mechanical strength requirements.

The glass fibers 7 in the exemplary embodiment of Figure 1 are connected to a transmission element 8, for example a conventional transponder, which may be disposed on the implant 1 itself or remote from the implant 1 in the interior of the patient's body or else on the surface of the patient's body; it may in this case also be an optical element, which can receive and emit light, for example a small parabolic mirror, a lens or the like. In the exemplary embodiment of Figure 1, all the glass fibers 7 disposed in the implant 1 are connected to the transmission element 8; in the exemplary embodiment of Figure 2, only some of the glass fibers are connected, while others serve

exclusively for reinforcing the implant 1. This can be chosen differently from case to case; in the extreme case, it is sufficient to connect a single glass fiber 7 in the implant 1 to such a transmission element 8.

5

The transmission element 8 has a corresponding associated transmission element 9, which is connected to the measuring device 11 via a line 10. Signals can be exchanged between the transmission elements 8 and 9; 10 these may be electrical signals, optical signals or mechanical signals (ultrasound); all that is important is that electromagnetic energy is transmitted from the transmission element 8 into the glass fiber and, if appropriate, from the glass fiber into the transmission 15 element 8 and is converted in the transmission element 8 into signals which can then be passed in any desired way to the transmission element 9, and consequently to the measuring device 11. If the transmission element 8 is disposed in the interior of the body, the 20 transmission elements 8 and 9 can exchange in particular an electromagnetic radiation with a wavelength of between 650 and 1000 nanometers; this electromagnetic radiation can penetrate the body tissue to a certain depth and can consequently establish a 25 signal connection between the two transmission elements 8 and 9, to be precise both in the inward radiating direction and in the outward radiating direction.

The radiation coupled into the glass fiber 7 in this 30 way is carried in the glass fiber 7 and changed by the latter itself or by a sensor member 12 connected to it, to be precise in a way dependent on the data relating to the physical state of the glass fiber 7, the sensor member 12 or the environment. The radiation then sent 35 in the return direction from the glass fiber 7 to the transmission element 8 is correspondingly changed, and this change can be detected by the measuring device 11, which consequently receives feedback on changes of the

physical state of the glass fiber, of the sensor member 12 and/or of the environment.

5 The possibilities for affecting the electromagnetic radiation fed into the glass fiber 7 are many and varied; changes in length, deformations, mechanical tensile stresses, forces, vibrations, pressures, angles of rotation, electric or magnetic field strengths, currents, temperatures, moisture, ionizing radiations
10 or the concentration or presence of chemical substances can be determined in this way; this is just a selection of the possible physical states that can be detected in this way. Some examples of the influencing of the electromagnetic radiation in a glass fiber are
15 discussed below on the basis of Figures 5 to 10.

In Figure 5, a detail of a glass fiber 7 is represented; provided in this glass fiber are various regions 13, 14, 15, which are spaced apart from one another in the longitudinal direction and in which
20 periodic changes of the refractive index occur in the longitudinal direction of the fiber. These can be produced for example by irradiating a quartz glass fiber, doped for example with germanium dioxide, with
25 ultraviolet light of 240 nm wavelength via a microlithographic mask. This produces in each region 13, 14, 15 an arrangement of a Bragg grating, the periodicity, and consequently the grating constant, being chosen differently in different regions 13, 14,
30 15.

At each of these Bragg gratings, a quite specific wavelength is reflected by interference radiation; this wavelength is dependent on the periodicity of the
35 grating, and consequently also changes when the latter changes periodicity. Such changing of the periodicity or grating constant may take place due to outside influences, for example strain of the glass fiber,

bending of the glass fiber, heating, etc. Since only radiation of a specific wavelength is reflected in each region 13, 14, 15, it is possible to ascertain immediately from the wavelength of the reflected radiation at which region a reflection has taken place; furthermore, the shift of the wavelength provides information on changes of the grating spacings in these regions, that is to say for example information on the strain of the glass fiber in specific regions. This may be different in the regions 13, 14, 15; the measuring device can provide indications on the basis of the reflected radiation as to the magnitude of the strain in each of the regions 13, 14, 15. Consequently, in particular when a number of such glass fibers are used, exact information about the deformation of the implant 1 in the body is obtained, and thus for example about the progress of healing during the growing together of bone fragments. The strain caused by the forces exerted will be greatest when the bone fragments have not yet grown together, and it will keep decreasing as the healing progresses.

In the case of the exemplary embodiment of Figure 6, embedded in the glass fiber 7 in a specific region 16 are dye particles 17, which are induced to fluoresce by electromagnetic radiation entering the glass fiber 7. The radiation emitted in this way can be determined by the measuring device. Environmental influences, for example certain chemical substances in the environment of the region 16, can influence the fluorescence, for example the intensity of the fluorescence may be reduced or else the fluorescence extinguished entirely. In this way, the measuring device receives information on the presence of certain chemical substances in the environment of the region 16.

In the case of the exemplary embodiment of Figure 7, the glass fiber 7 is sheathed with a coating 18, which

prevents the electromagnetic radiation carried by the glass fiber 7 from emerging. This coating may react with chemical substances 19 in the environment and thereby undergo a transformation such that the emerging
5 properties of the electromagnetic radiation are changed in the region in which the chemical substance 19 is located, and in this way a change of the reflected radiation is again obtained in dependence on certain chemical substances 19 in the environment of the glass
10 fiber 7.

In the case of the exemplary embodiment of Figure 8, the ground-flat end 20 of the glass fiber 7 is opposite a likewise ground-flat end 21 of a piece of glass fiber
15 22, a very narrow gap 23 being produced between the ends 20 and 21; the gap width A may for example be of the order of magnitude of 50 mm. This arrangement forms a Fabry-Pérot interferometer and reflects radiation of a quite specific wavelength, which is
20 dependent on the gap width A. If the two ends 20 and 21 are shifted in relation to each other, a shift of the wavelength of the reflected radiation thus also occurs, and this can be detected with great sensitivity. It is also readily possible in this way
25 to detect for example strains of the implant, which are transferred to the glass fiber 7 and the piece of glass fiber 22.

In the case of the exemplary embodiment of Figure 9, a
30 similar arrangement is chosen, but an active layer 24 which changes its dimension, for example its volume, in dependence on environmental influences is inserted into the gap 23. This layer may be, for example, a porous structure which swells when liquid enters into the
35 pores. The gap width B changes as a result, and this leads to changing of the wavelength of the radiation reflected at the Fabry-Pérot arrangement.

The Fabry-Pérot arrangements of Figures 8 and 9 consequently form a sensor member 12 which is connected to the measuring device 11 via the glass fiber 7; in the case of the exemplary embodiments of Figures 5 to 7, on the other hand, the glass fiber 7 itself is a sensor element, so this is a case of glass fibers that are themselves sensor fibers.

10 In the case of the exemplary embodiment of Figure 10, a sensor member 12 in the form of a pressure sensor 25 is associated with the glass fiber 7. This comprises a flexible membrane 26, which is provided on one side with a reflective layer 27. If this pressure sensor 25 is disposed at the end of a glass fiber 7, the
15 electromagnetic radiation reflected back into the glass fiber 7 changes with the deformation of the membrane 26, which takes place pressure-dependently, and consequently a measure of the pressure at the end of the glass fiber 7 is again obtained.

20

In the case of the exemplary embodiment of Figures 1 and 2, glass fibers 7 which are led out from the implant 1 are connected directly or indirectly to the measuring device 11.

25

This is carried out in a similar way in the case of the embodiment according to Figure 3, which is set up in a way similar to that of Figure 1 and in which identical parts are designated by corresponding reference
30 numerals; the connection of the transmission element 8 to the measuring device 11 is symbolized in the case of the exemplary embodiment in Figure 3 by a line 10, which may be a physical line or a transmission link without a line.

35

Additionally provided in the case of this embodiment is a radiation source 29, which is connected to one or more glass fibers 30, which are embedded in the

synthetic material 6 of the implant 1. In the exemplary embodiment of Figure 3, only one such glass fiber 30 is represented, which is connected directly to the radiation source 29; this is to be considered only
5 as a schematic representation. It is also possible here for a number of glass fibers 30 to be provided which, in a way similar to how the glass fibers 7 are connected to the measuring device, are connected for their part to the radiation source 29, that is to say
10 via transmission elements which could be disposed in the body or outside it, etc. The radiation source 29 can feed into the glass fibers 30 an electromagnetic radiation, which emerges in the interior of the implant 1 and produces there a direct influence on the
15 environment, for example heating-up of the surrounding synthetic material 6 or else additional hardening by increased polymerization or else dissolution of polymerization bonds, etc. Many effects are conceivable here, dependent on the nature of the
20 synthetic material 6 used and on the nature of the electromagnetic radiation fed in. In any event, this fed-in electromagnetic radiation has the effect of influencing the physical data of the synthetic material 6 and possibly of the environment of the implant 1; for
25 example, the strength of the implant can be increased or reduced locally or over its surface area. The location where the effect occurs can be determined by corresponding arrangement of the glass fibers 30 in the implant 1; the type of effect can be determined by
30 corresponding selection of a specific radiation.

The radiation source 29 may be activated completely independently of the measuring device 13; however, it is particularly advantageous if, as represented in
35 Figure 3, associated with the radiation source 29 is a controller 31, which switches the radiation source 29 on and off in dependence on the measured data of the measuring device 11. For this purpose, the measuring

device 11 is connected to the controller 31 via a line 28.

If, for example, the measuring device 11 detects that
5 the strain of the implant 1 decreases in a specific
region, this is an indication that part of the force
transfer has been taken over by healing bone fragments;
the strength of the implant 1 can then be reduced by
dissolving part of the synthetic material 6 by feeding
10 in electromagnetic radiation into glass fibers 30, with
the result that the supporting function of the implant
1 is reduced in a way corresponding to the increase in
the stability of the bone connection. Consequently,
optimum adaptation of these parameters to each other is
15 possible; it is also beneficial for the healing if the
bone connection is increasingly subjected to loading as
the healing process proceeds.

In the case of the exemplary embodiment of Figure 3,
20 the introduction of the radiation generated by the
radiation source 29 takes place via glass fibers 30,
which are different from the glass fibers 7 of the
measuring device.

25 It is also possible to perform both the measurement of
the data relating to the physical state and the
feeding-in of electromagnetic radiation via the same
glass fibers 7; this is schematically represented in
Figure 4. For this purpose, an optical switch 33,
30 which selectively permits a connection of the glass
fibers 7 to the measuring device 11 or the radiation
source 29, is connected between the transmission
element 8 on the one hand and the measuring device 11
and the radiation source 29 on the other hand. This is
35 symbolically indicated in Figure 4 by the double-headed
arrow C. Switches of this type are available in
various ways; they may be mechanical switches, which
for example displace a glass fiber between two

coupling-in points, or else switches which operate electromagnetically, piezoelectrically or thermally; a large number of different switches that can be used for this purpose are known here to a person skilled in the art.

The optical switch 33 may optionally also be automatically actuated, ensuring as a result that for example alternately a measurement of the physical state is performed via the glass fiber 7 and radiation energy is fed in for influencing the environment of the glass fiber.

PATENT CLAIMS

1. Medical implant system with an implant (1) made of a composite material in which glass fibers (7) are embedded, characterized in that a sensor element which is embedded in the implant (1) and comprises at least one of the glass fibers (7) is connected to a measuring device (11) which determines a physical property of the sensor element or its environment and changing of this property.
2. Implant system according to Claim 1, characterized in that the glass fibers (7) are embedded in the composite material as mechanical reinforcement.
3. Implant system according to one of the preceding claims, characterized in that the glass fibers (7) are arranged in the form of a woven fabric, a knitted fabric or a non-woven fabric.
4. Implant system according to one of the preceding claims, characterized in that the glass fibers (7) are distributed in the composite material over the entire extent of the implant (1).
5. Implant system according to one of the preceding claims, characterized in that the measuring device (11) feeds electromagnetic radiation into the sensor element and determines physical properties of the sensor element or of its environment from the type of radiation that passes through and/or is reflected.
6. Implant system according to Claim 5, characterized in that the glass fiber (7) of the sensor element is provided with a radiation-reflecting coating (18).

7. Implant system according to one of the preceding claims, characterized in that the sensor element substantially consists of the glass fiber (7) forming a sensor fiber.
- 5 8. Implant system according to Claim 7, characterized in that at least one region (13, 14, 15) acting as a Bragg grating is incorporated in the sensor fiber.
- 10 9. Implant system according to Claim 7, characterized in that there is embedded in the sensor fiber a substance (17) which is induced to fluoresce by the fed-in electromagnetic radiation and the
15 fluorescent properties of which undergo changes under the effect of the chemical environment outside the sensor fiber.
- 20 10. Implant system according to Claim 6 and 7, characterized in that the radiation-reflecting coating (18) consists of a substance which changes the reflection behavior for the electromagnetic radiation in the sensor fiber under the effect of the chemical environment (19) outside the sensor
25 fiber.
- 30 11. Implant system according to one of Claims 1 to 5, characterized in that the sensor element comprises the glass fiber (7) and a further sensor member (12), which is connected to the measuring device (11) via the glass fiber (7).
- 35 12. Implant system according to Claim 11, characterized in that the sensor member (12) is a pressure sensor (25) with a flexible membrane (26) and a mirror element (27) which can be moved by the latter and reflects the electromagnetic radiation fed into the glass fiber (7) differently according to position.

13. Implant system according to Claim 11, characterized in that the sensor member (12) is a Fabry-Pérot interferometer.
- 5
14. Implant system according to Claim 13, characterized in that the Fabry-Pérot interferometer is formed as a thin-film interferometer (21, 22, 24) that is brought into contact onto and at the end (20) of the glass fiber (7) and the active film (24) of which undergoes dimensional changes under the influence of the environment.
- 10
15. Implant system according to Claim 13, characterized in that the Fabry-Pérot interferometer comprises two glass fibers (7, 22) with polished end faces (20, 21), the spacing (B) between which can be changed by environmental influences.
- 15
16. Implant system according to one of the preceding claims, characterized in that the glass fiber (7) of the sensor element is connected directly to the measuring device (11).
- 20
17. Implant system according to Claim 16, characterized in that the measuring device is a microcontroller that is capable of being implanted in the body.
- 25
18. Implant system according to one of Claims 1 to 15, characterized in that the glass fiber (7) is connected to a transducer (8), which exchanges signals with the measuring device (11) without a physical connection.
- 30
19. Implant system according to Claim 18, characterized in that the transducer (8) is capable of being implanted in the body.
- 35

20. Implant system according to Claim 18 or 19, characterized in that the transducer (8) is a transponder.
- 5 21. Implant system according to Claim 18 or 19, characterized in that the transducer is a light source with which a light receiver is associated.
- 10 22. Implant system according to Claim 21, characterized in that the light source emits electromagnetic radiation in the range between 650 and 1000 nm.
- 15 23. Implant system according to one of the preceding claims, characterized in that associated with the measuring device (11) is a radiation transmitter (29), which transports radiation into the interior of the implant (1) via a glass fiber (7; 30) in the implant (1).
- 20 24. Implant system according to Claim 23, characterized in that the transport of the radiation takes place via the glass fiber (7) of a sensor element.
- 25 25. Implant system according to Claim 23, characterized in that the transport of the radiation takes place via a glass fiber (30) which is embedded in the implant (1) in addition to the glass fiber (7) of a sensor element.
- 30 26. Implant system according to one of Claims 23 to 25, characterized in that the wavelength and intensity of the transported radiation are chosen such that the radiation induces mechanical and/or material changes in the composite material of the implant.
- 35 27. Implant system according to one of Claims 23 to 26, characterized in that associated with the measuring device (11) and the radiation transmitter (29) is a

controller (31), which activates the radiation transmitter in dependence on the measured values of the measuring device (11).

ABSTRACT

In the case of a medical implant system with an implant made of a composite material in which glass fibers are embedded, to obtain information on physical states of the implant in its environment it is proposed that a sensor element which is embedded in the implant and comprises at least one of the glass fibers is connected to a measuring device which determines a physical property of the sensor element or its environment and changing of this property.

tran 1264 from tran 0840: Hoeger A 100 584 u: pr doc, mjlw, Jul 5, 2005.

FIG.1

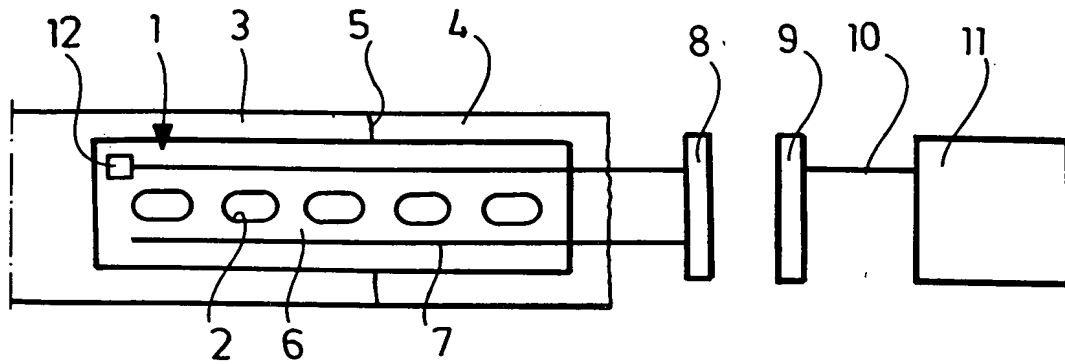


FIG.2

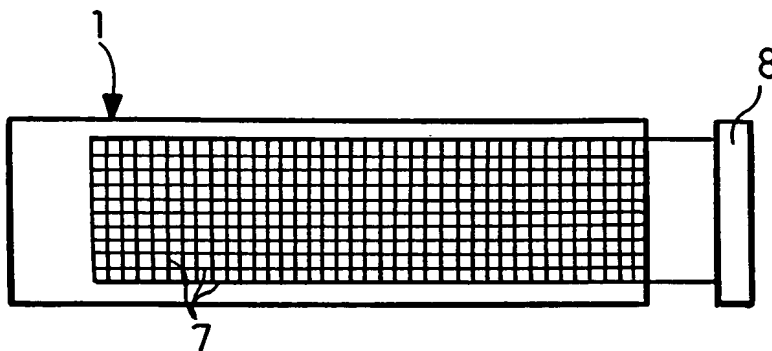


FIG.3

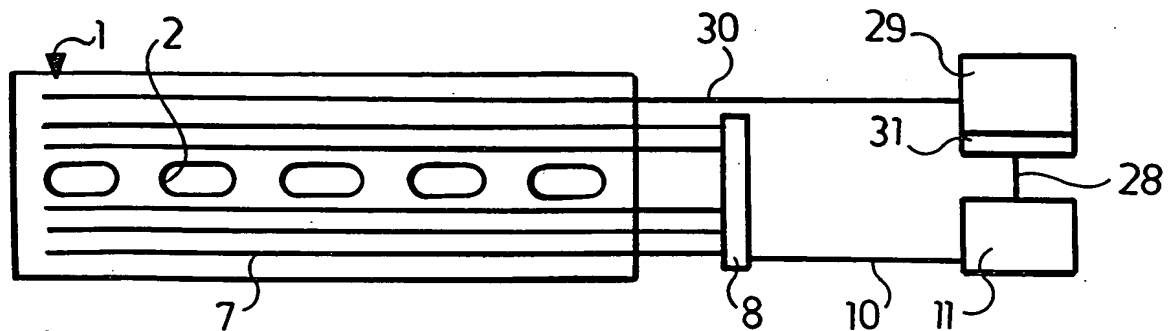


FIG.4

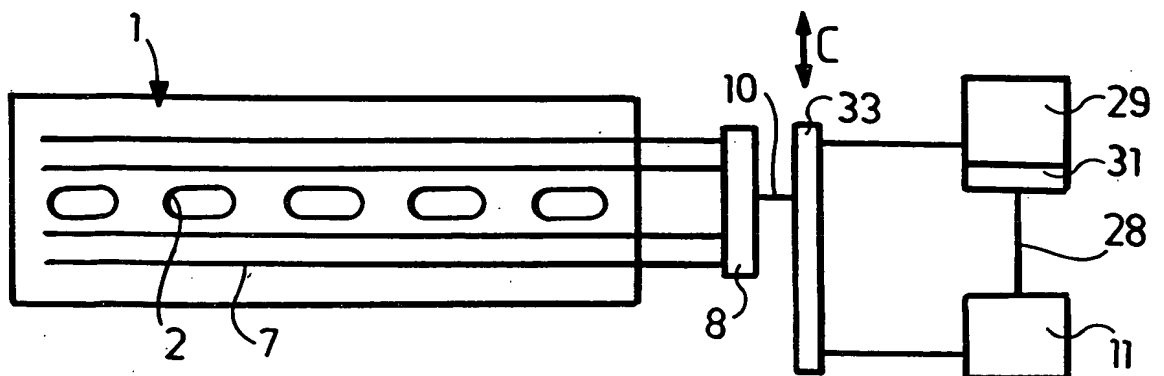


FIG.5

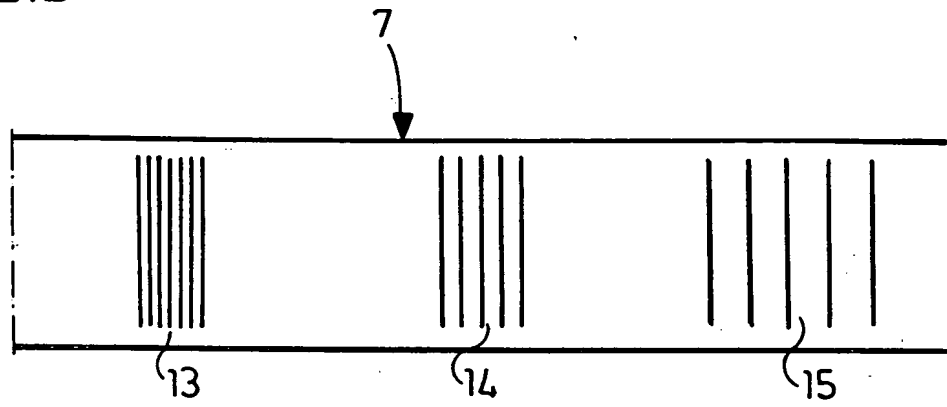


FIG.6

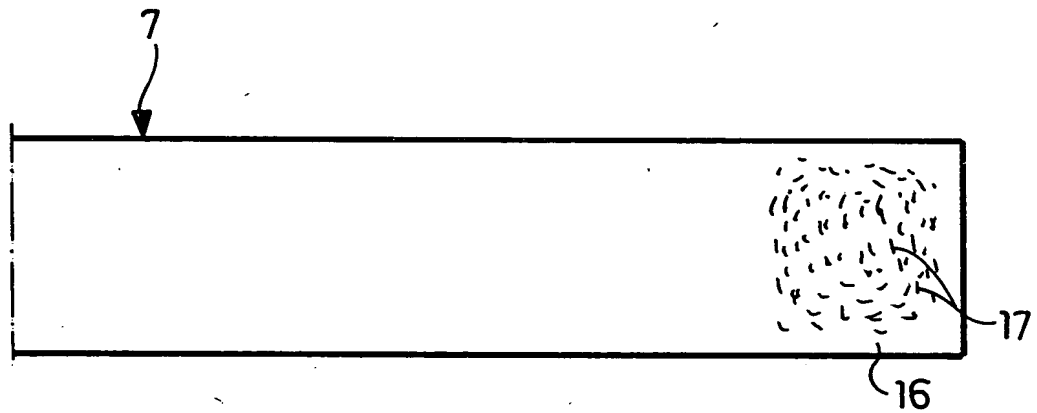


FIG.7

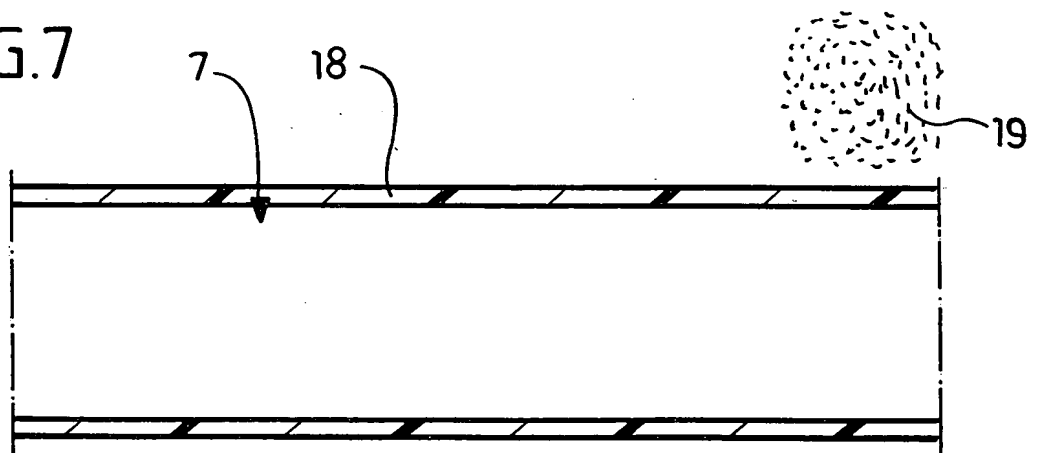


FIG.8

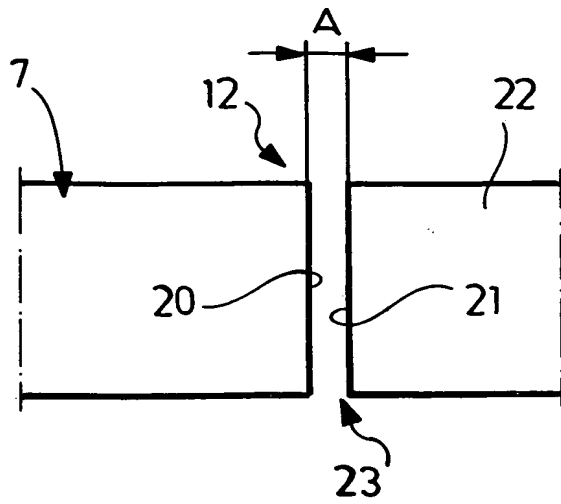


FIG.9

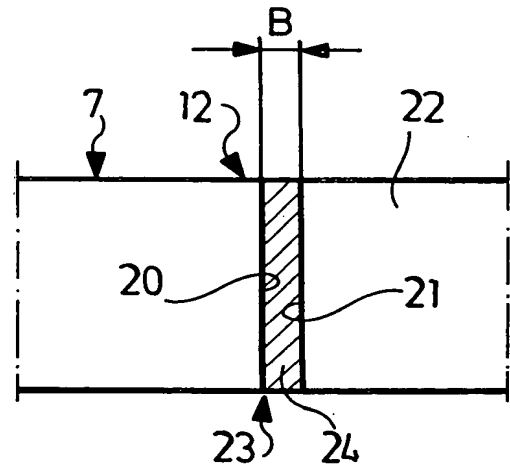


FIG.10

